

USER MANUAL

MNPG366-02 Edition 04/07/2022

CV2S2000
Professional
applicator with two
solenoids

I.A.C.E.R. Srl

www.itechmedicaldivision.com

Introduction

The **CV2S2000** device is a professional two-solenoid applicator for low-frequency magnetotherapy. It is easily adaptable to any area of the body thanks to the presence of the therapeutic elastic tape.

The device is classified as class I, in accordance with rule 1 (4.1) referred to in Annex VIII of Regulation (EU) 2017/745 of the European Parliament and of the Council, dated 5 April 2017, relating to medical devices.

Basic UDI-DI: 8019781PEMFLFAPPP8


UDI-DI: 08019781472076

Technical data

Technical specifications:

- *Applicator size: diameter 11 cm + elastic tape of 115 cm;*
- *Cable length: 184 cm;*
- *2 professional solenoids;*
- *1 connection cable;*
- *Compatible with MAG2000 and LaMagneto series models.*

Labelling


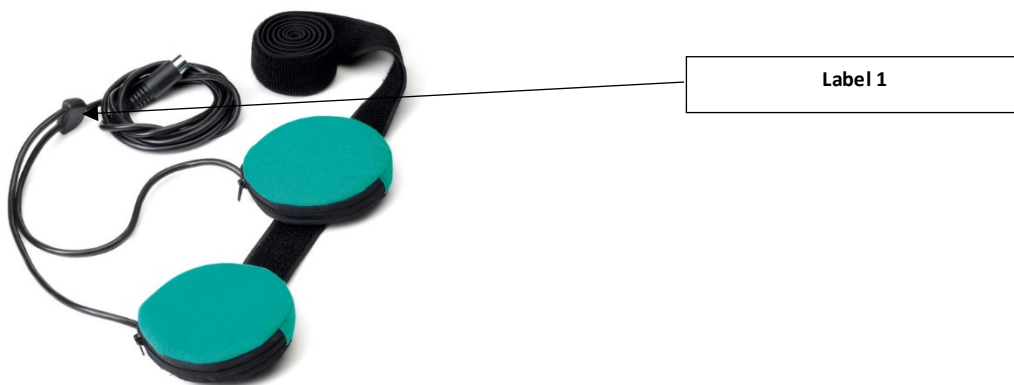


Label 1











29x18.7mm

Label 2 - (Cable label)



Symbols:

Symbol	Meaning
	Manufacturer's logo.
	In compliance with regulation (EU) no. 2017/745

Symbol	Meaning
	Manufacturer data.
	Date of manufacture (MM-YYYY).
	Follow the instructions for use.
	Medical device.
	WEEE directive for the disposal of electronic waste.
	Type BF applied part.
	Allowed temperatures (storage temperatures, on packaging).
	Relative humidity (relative humidity of storage, on packaging).

Transport and storage

There are no special care instructions for transport. For storage, the equipment is protected up to the following environmental conditions:

room temperature from +5 to + 40°C

relative humidity from 15 to 93%

Instructions for use

Instructions for using CV2S2000

Follow the instructions in the User Manual supplied with the device in your possession.

Follow the Instructions given in the user manuals of the products of the MAG2000 or LaMagneto series.


How to take care of CV2S2000

Cleaning the CV2S2000

To clean the CV2S2000 device, it is recommended to disconnect the professional two-solenoid applicator from the device before carrying out any operation. Clean the fabric with a cloth dampened with simple water and neutral soap and wait for it to dry completely before reusing the two-solenoid applicator for a therapy session.

Information for disposal



The product is subject to the WEEE legislation (presence on the label of the symbol ) relating to separate waste collection: to dispose of the product, use special areas equipped for the collection of electronic material by contacting the competent authorities of your country or the manufacturer directly.

Maintenance and Support

The device does not require any particular routine maintenance. Please contact the manufacturer to provide for a check of the functionality of the device, every two years. The manufacturer is the sole entity authorized to provide technical support for the CV2S2000 applicator. Should you need technical support, please contact:

I.A.C.E.R. S.r.l.

Via Enzo Ferrari, 2 • 30037 Scorzè (VE)

Ph. 041.5401356 • Fax 041.5402684

Warranty

CV2S2000 is covered by a 2-year warranty starting from the date of purchase. The warranty shall lapse in case of tampering, neglect and inappropriate use of the applicator and in case of any intervention carried out by personnel who is not authorized by the manufacturer or by the authorized dealer.

Incident reporting

In compliance with the provisions of Regulation (EU) 2017/745, the manufacturer places the need to report any serious accident in relation to the device to the attention of the user.

The report must be addressed:

- *to the device manufacturer:*

I.A.C.E.R. Srl
Via Enzo Ferrari 2 – 30037
Scorzè (VE) ITALY
Tel. +39 041 5401356 – Fax +39 041 5402684
e-mail: iacer@iacer.it

All rights reserved. CV2S2000 and the logo  are the exclusive property of I.A.C.E.R. Srl and are registered trademarks



I.A.C.E.R. S.r.l.

Via Enzo Ferrari 2 - 30037, Scorzè (VE) – Italy
Tel.: (+39) 041 540 13 56 | Email: iacer@iacer.it

www.itechmedicaldivision.com

Share Capital: € 1.000.000 fully paid-up
Tax Code / VAT Number: IT 00185480274
Certified email: iacer@pec.it | SDI: SUBM70N